

Primeva Labs
support@primevalabs.com
1001 E Playa Del Norte Dr, Unit
3110 Tempe, AZ 85288



COC# 145688
Lab # 212248
Date Rec'd 8/20/2026
Report Issued 9/8/2026

Compound Tesamorelin
Label Claim 20 mg

Project: 212248
Batch/Lot: PV-2608-TESA20-01


Certificate of Analysis

<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>LOQ</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
Peptide Analysis							
Chromatographic purity	>99.9	%	1		HPLC-UV/MS	8/26/2026	
Tesamorelin	21.5	mg	.1	107.4	HPLC-UV-MS	8/26/2026	218949-48-5
Mass Spectral Match	ID Confirmed				HPLC-UV-MS	8/26/2026	
Microbiology							
Endotoxins LAL Clot	<0.5	EU	.5		USP 85	8/28/2026	
FDA Critical Metals							
Arsenic	ND	µg	0.50		USP 233	9/4/2026	7440-38-2
Cadmium	ND	µg	0.10		USP 233	9/4/2026	7440-43-9
Mercury	ND	µg	0.20		USP 233	9/4/2026	7439-97-6
Mercury	ND	µg	0.20		USP 233	9/4/2026	7439-97-6

The data presented are solely from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged. Data is solely for the use of the recipient as shown. No other use is authorized. Methods shown reference current Krause Analytical SOPs
ND - Not detected LOQ - limit of quantification OC - outside of calibration
Copyright © 2026 Krause Analytical LLC. All rights reserved.

Respectfully submitted,

Mark C. Krause
Laboratory Director

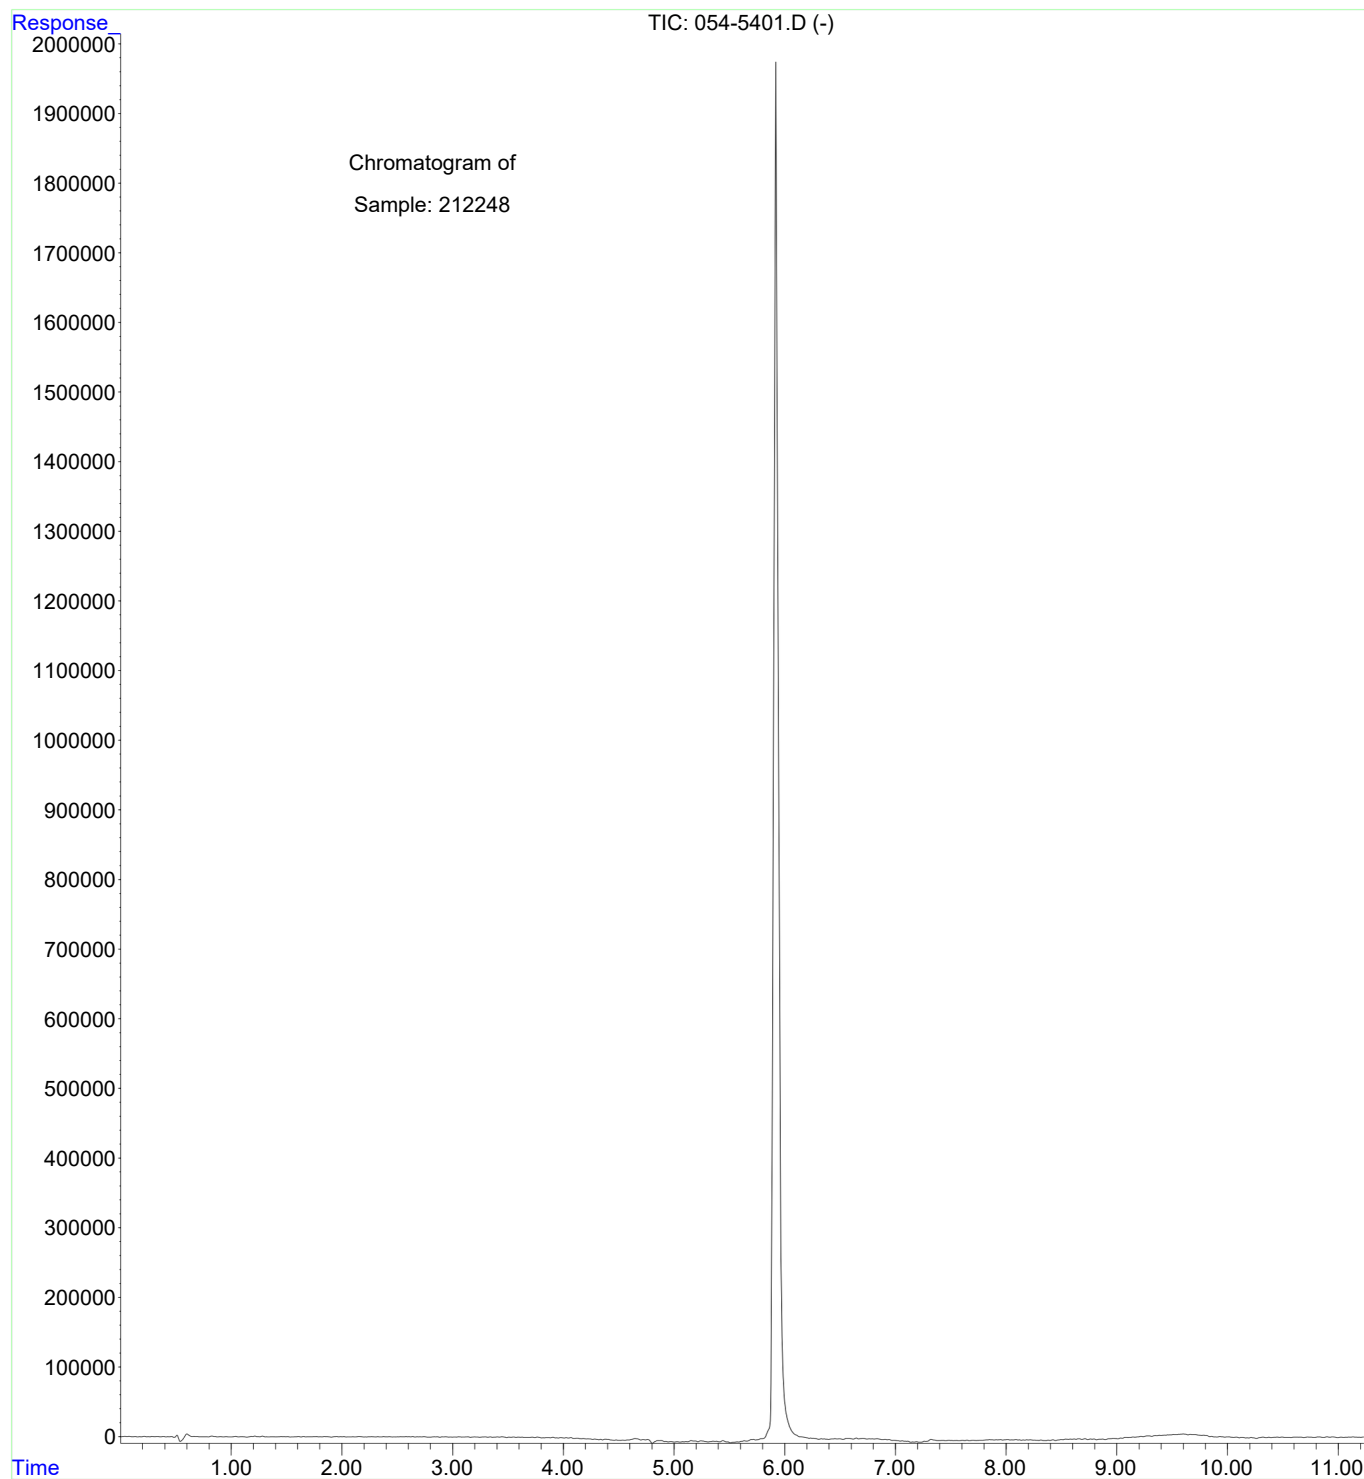

Sample Report:

1: (Time: 0.30) Combine (13:19-(7:10+30:33))

1:MS ES+
7.6e+006